


Data file: D:\CHEM32\1\DATA\240620\20240620 2024-06-20 11-09-38\  
 24060037Final.D  
 Sample name: 24060037Final  
 Description: Mobile phase:Buffer A:0.1%TFA in H2O  
Buffer B:0.1%TFA in ACN  
 Gradient:33-43% B in 20min , Flow rate:1.0ml/min  
 Column:Unitary C18, 4.6\*150mm, Sum 100A  
 Instrument:Agilent HPLC 1100

Instrument: 1100 Location: 46  
 Injection date: 2024/6/20 11:42:22 Injection: 1 of 1  
 Last changed: 2024/6/20 12:29:44 Injection volume: 10.000  
 Acq-operator: SYSTEM

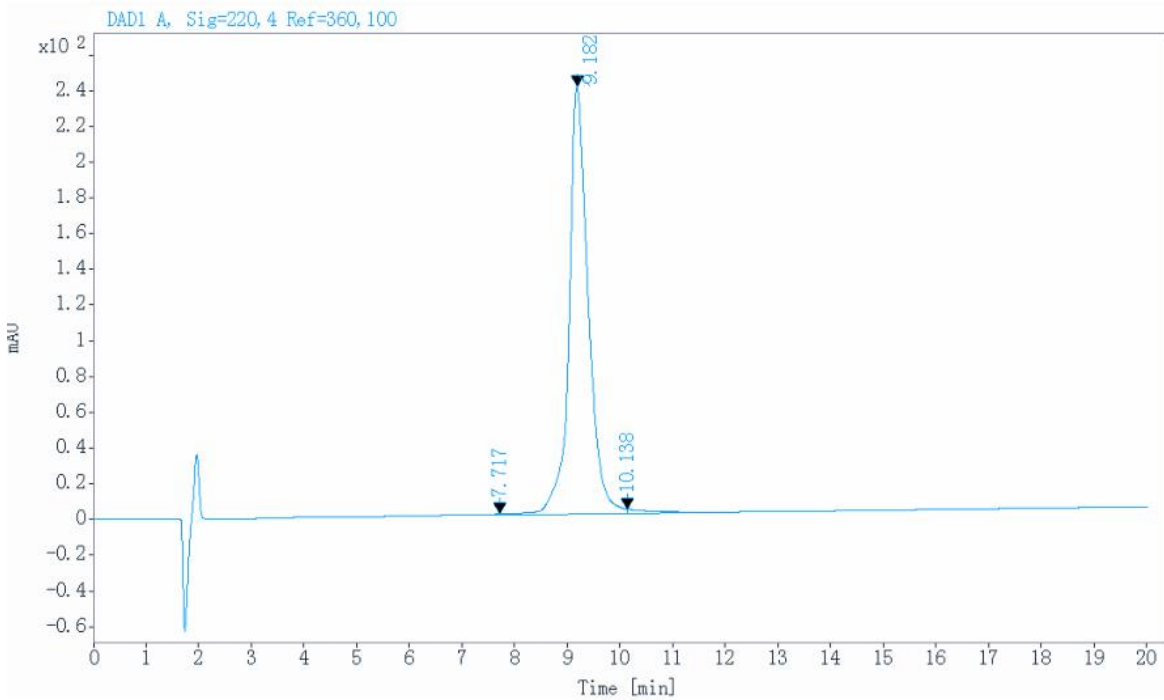

Signal: DAD1 A, Sig=220, 4 Ref=360, 100

RT[min]	Type	Width[min]	Area	Height	Area% Name
7.717	FM	0.2882	8.6914	0.5027	0.1421
9.182	MF	0.4211	6047.5317	239.3288	98.8936
10.138	FM	0.4576	58.9644	2.1478	0.9642
Sum			6115.1875		